

FIG. 1

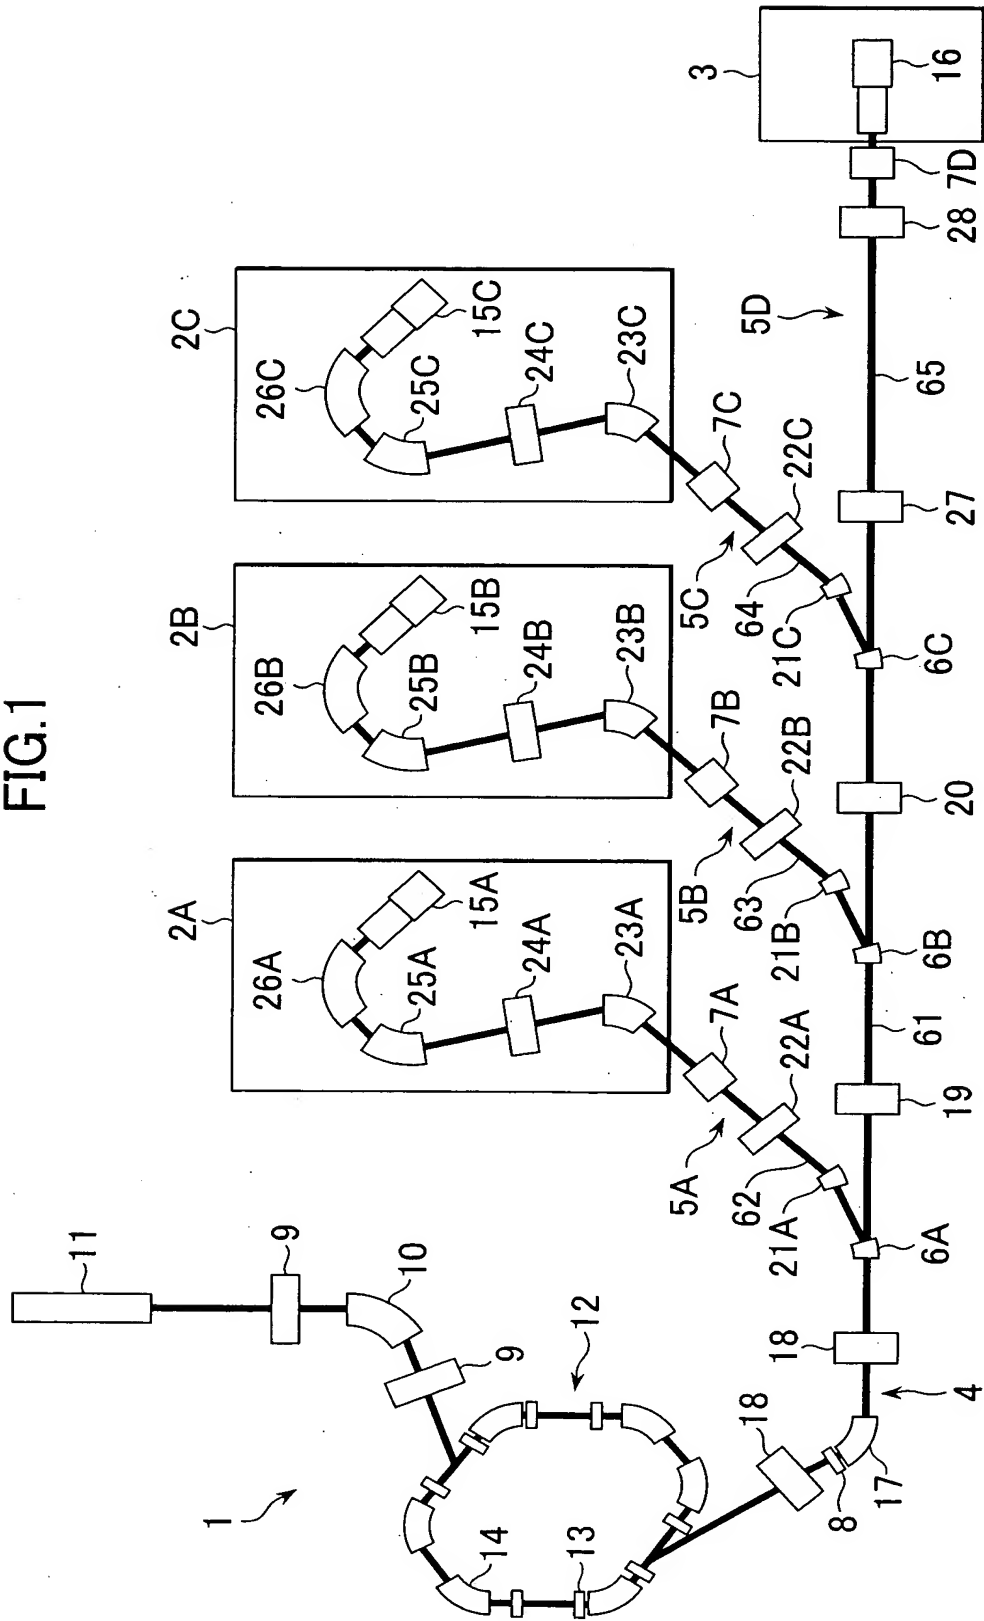


FIG.2

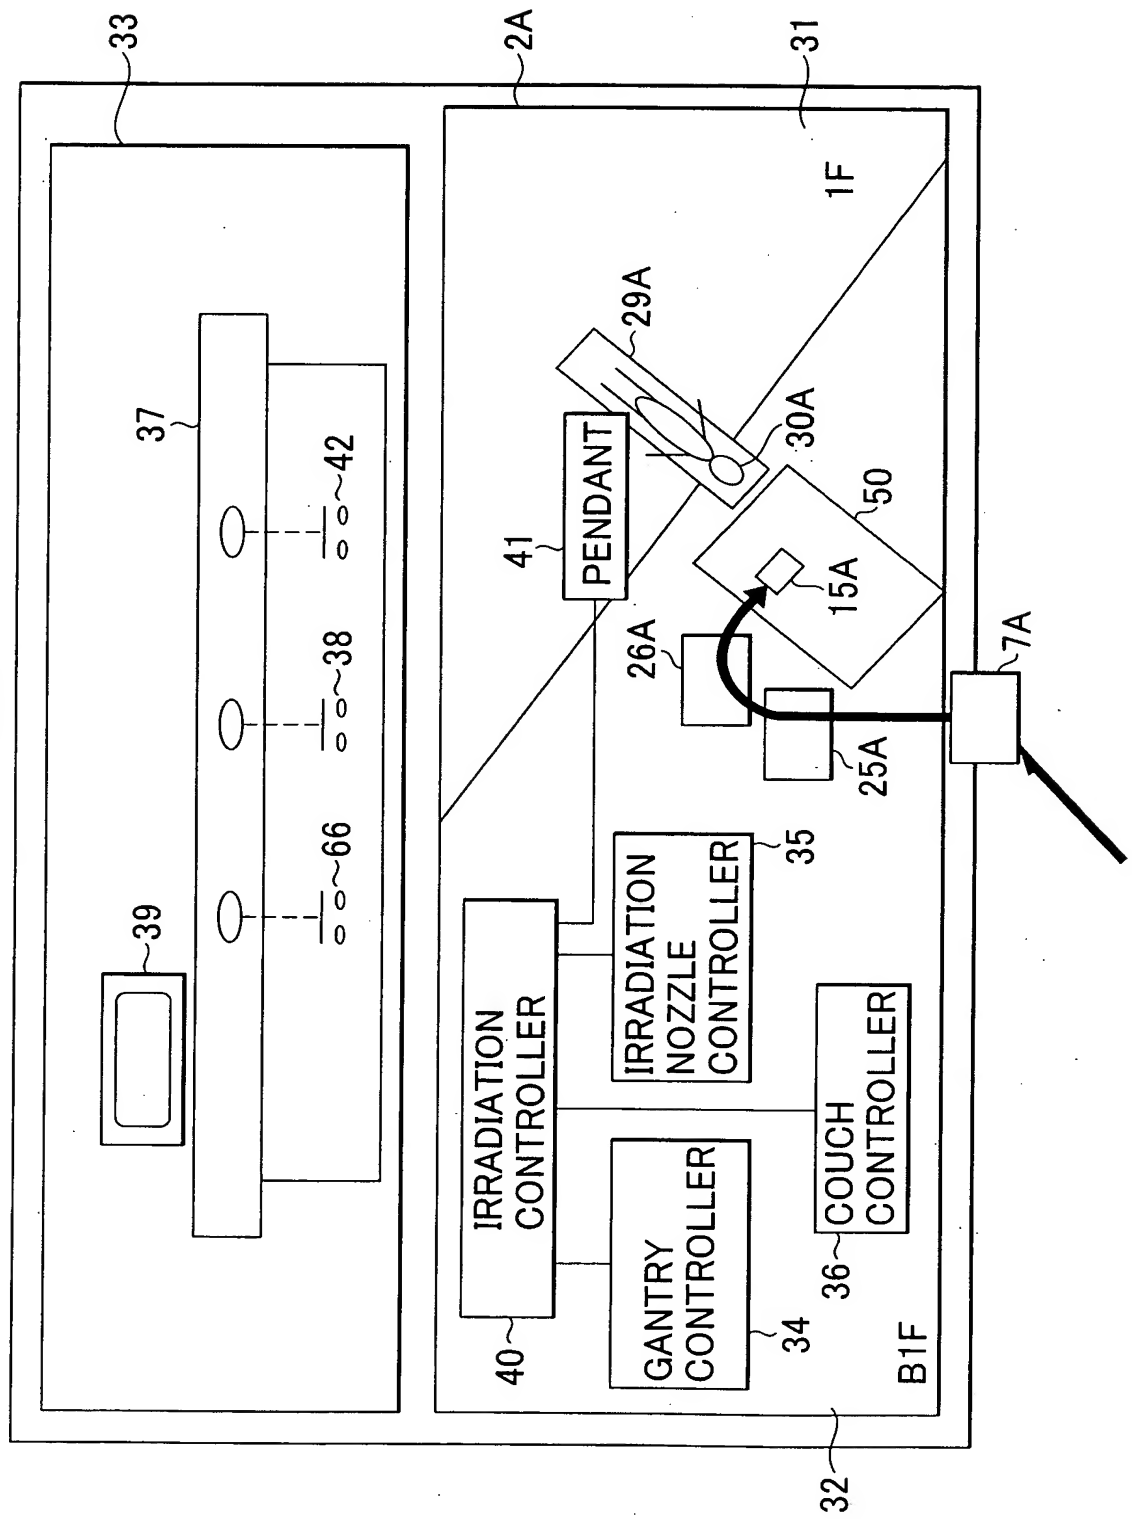


FIG.3

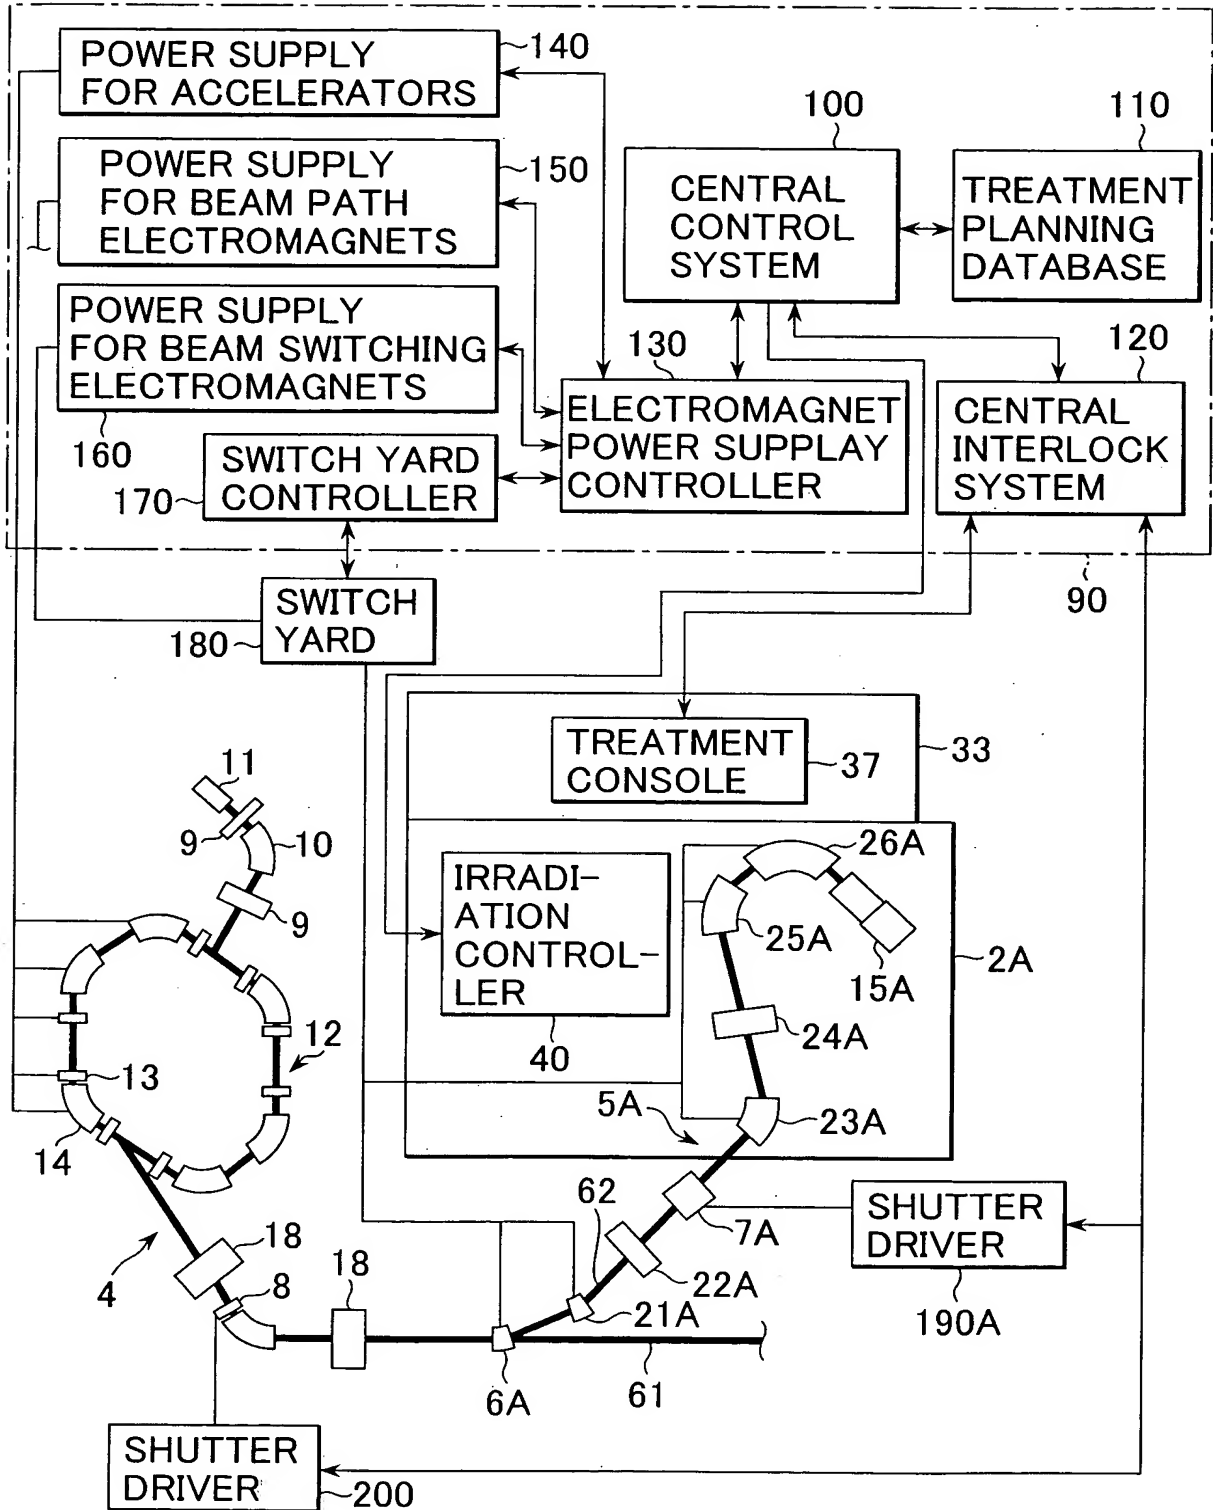
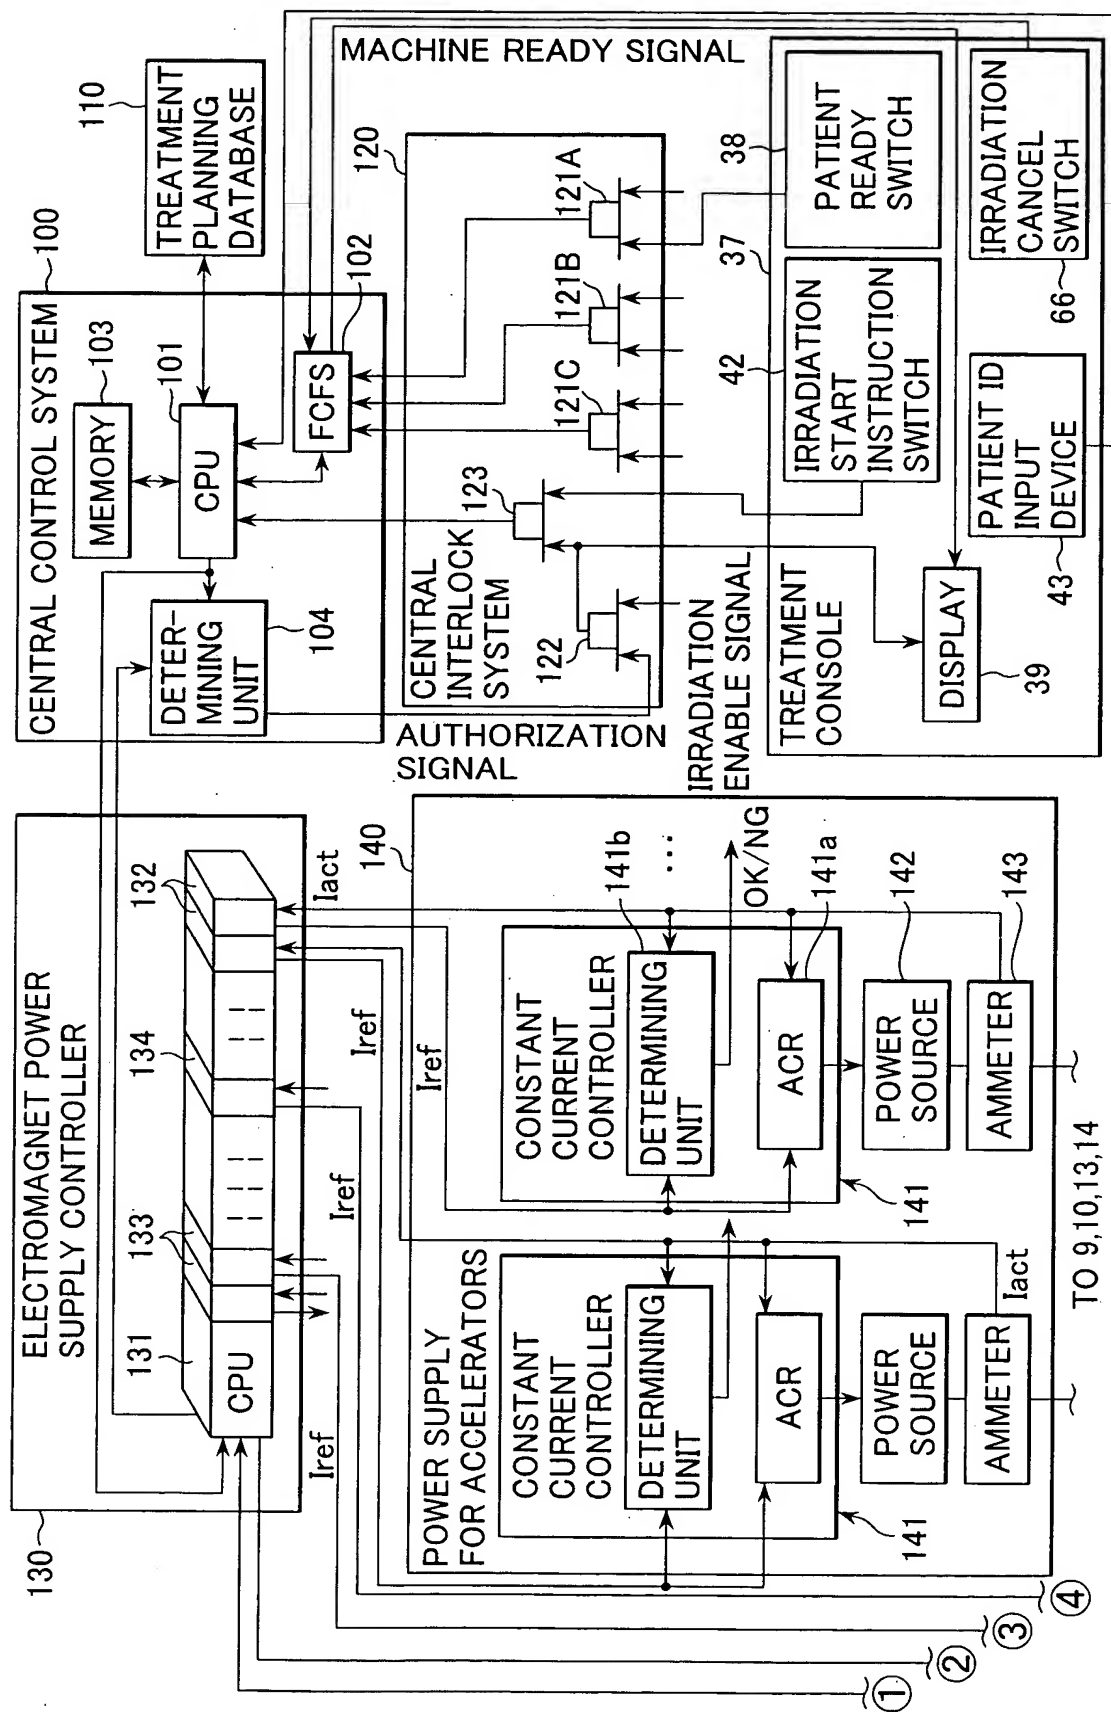


FIG.4



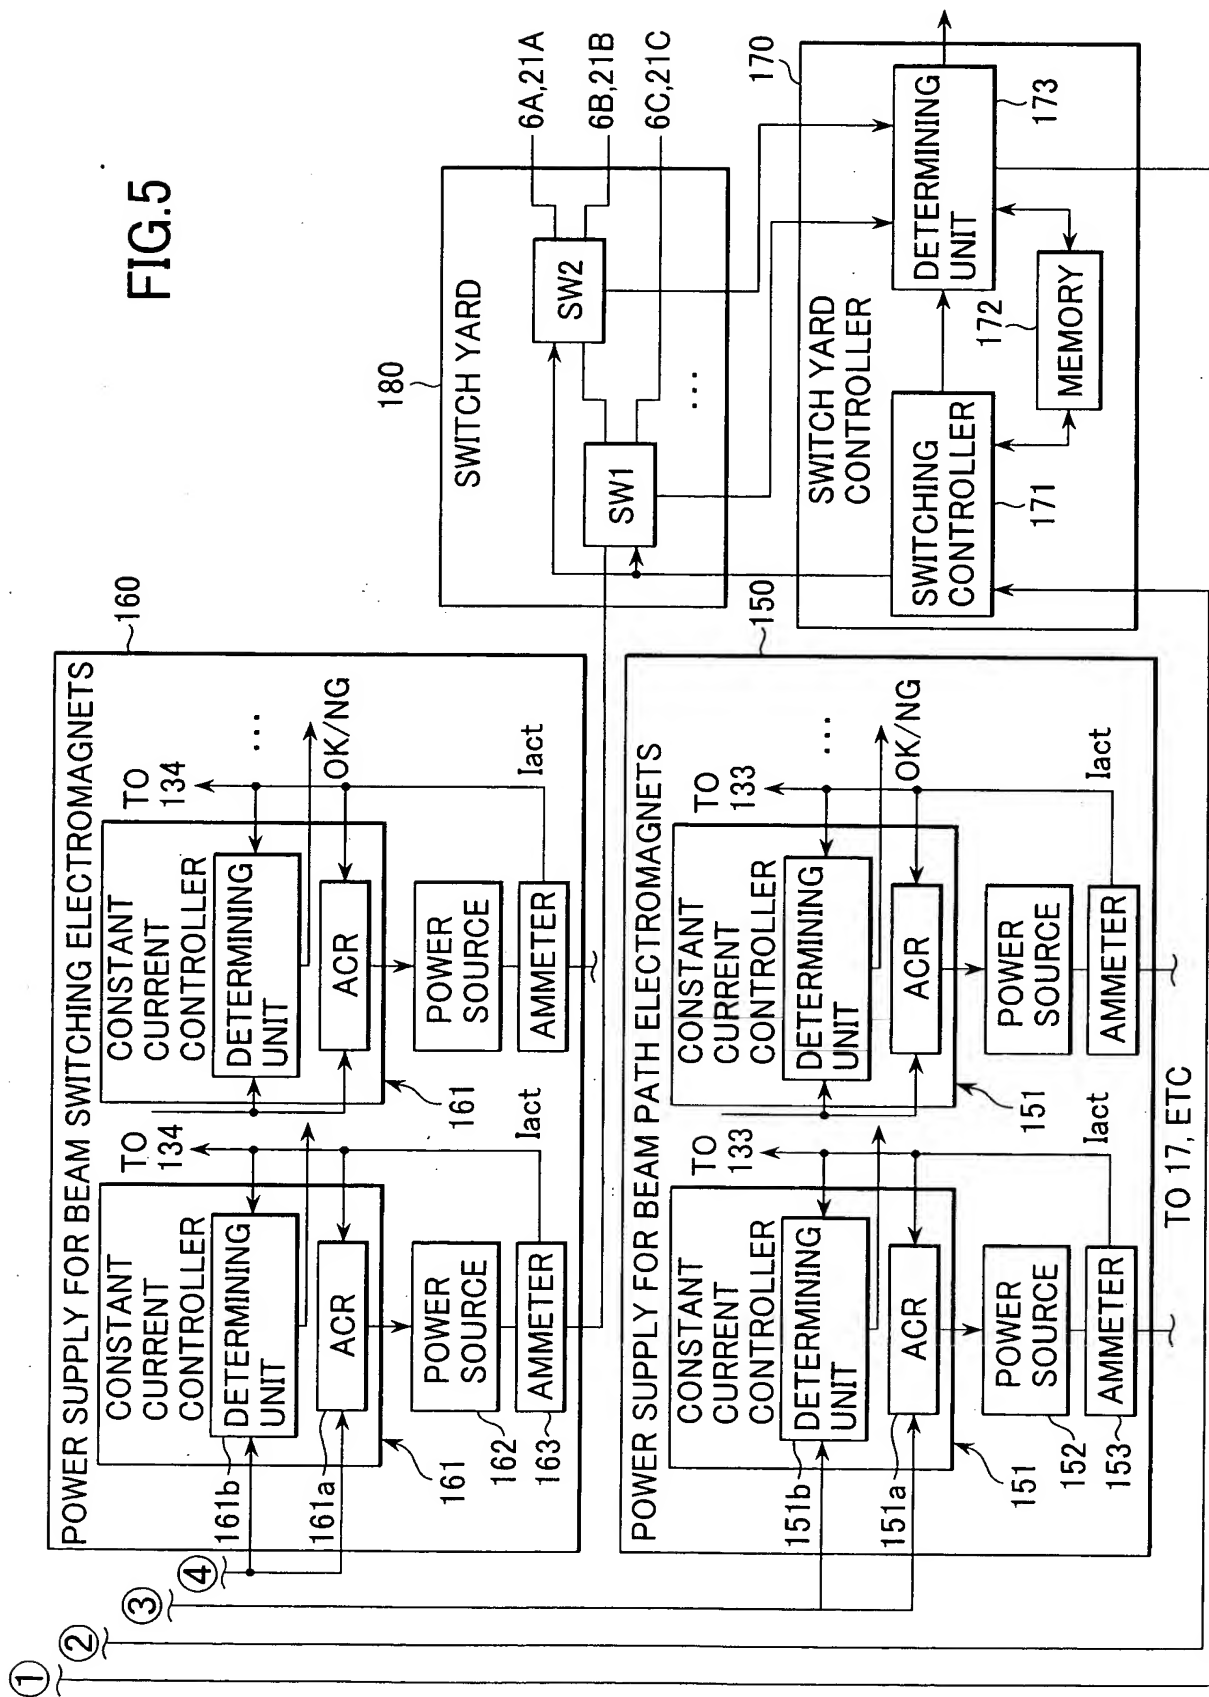


FIG.6

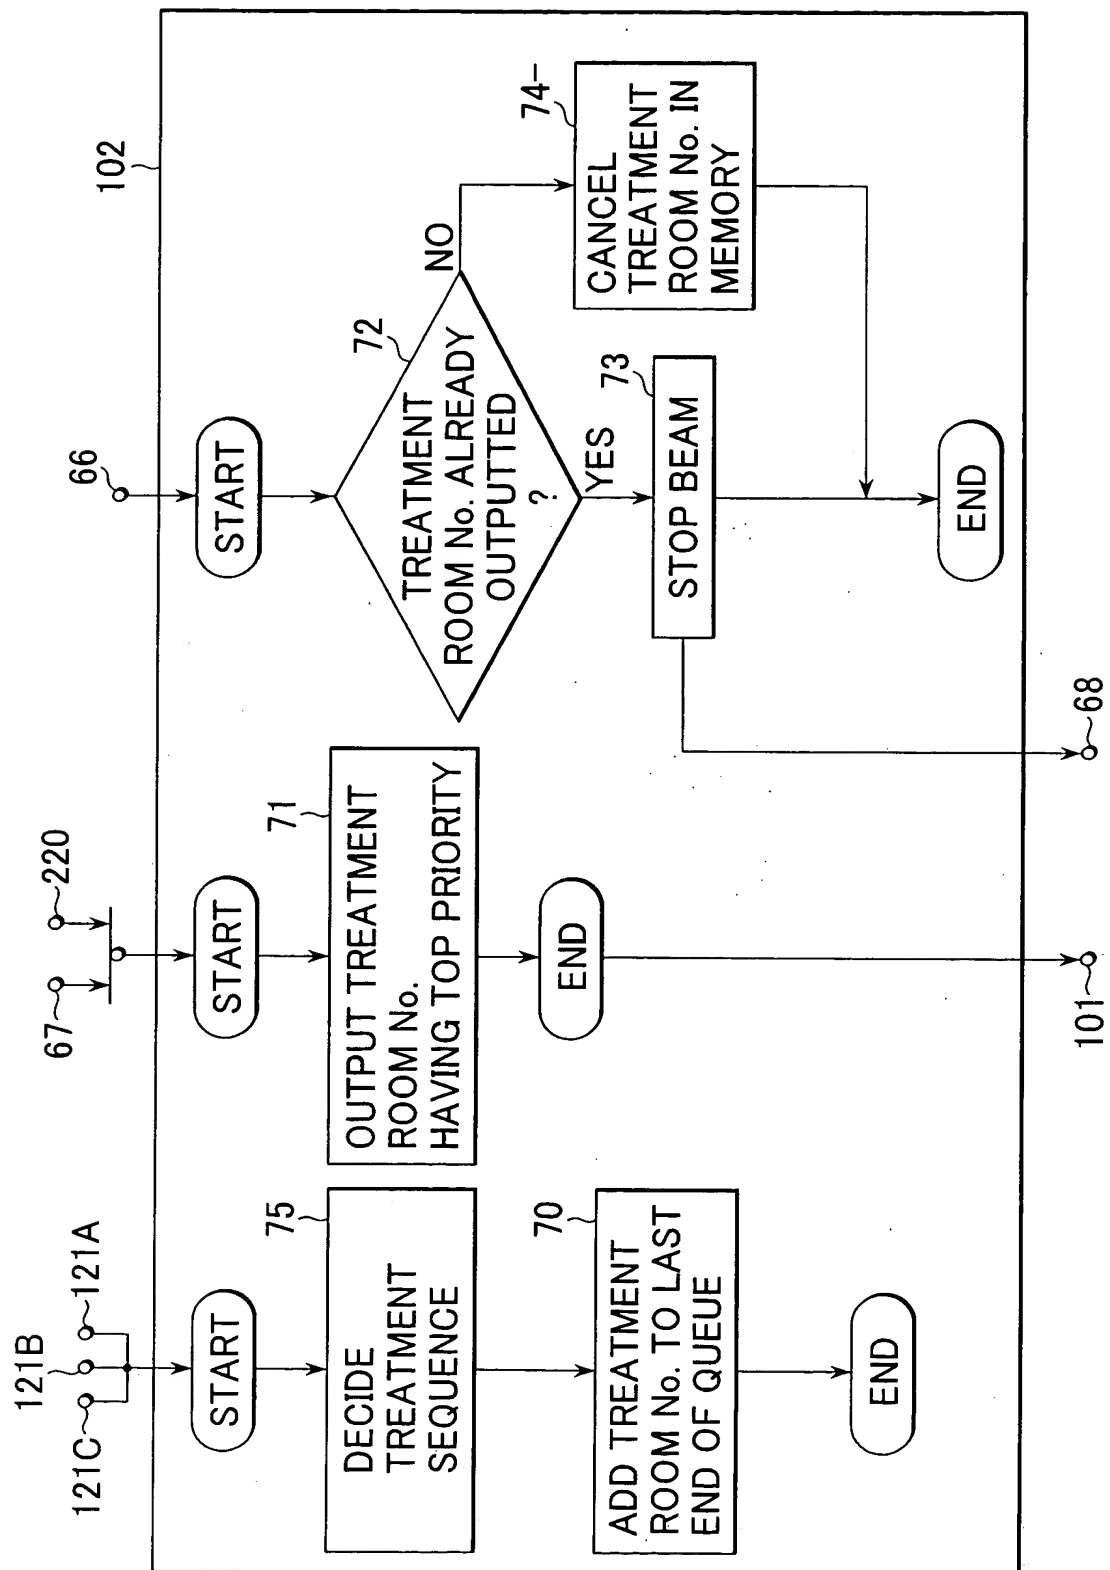


FIG.7

PATIENT DATA

PATIENT ID No.	DOSE	(TREATMENT ROOM No.)	ENERGY	.....
650098	....	(No.1)	70Mev	.....

# FIG.8

GB : BENDING ELECTROMAGNET

GQ : QUADRUPOLE ELECTROMAGNET

ENERGY (MeV)	COMMON						
	BEFORE ACCELERATION		SYNCHROTRON			AFTER ACCELERATION	
	GB10	GQ9	GB14	GQ13	GQ13	GB17	GQ18
70	...	...	Pattern 70			...	...
80			Pattern 80			...	...
90			Pattern 90			...	...
⋮			⋮			⋮	⋮
⋮			⋮			⋮	⋮
⋮			⋮			⋮	⋮

ENERGY (MeV)	No.1 TREATMENT ROOM 2A		No.1 to No.2	No.2 TREATMENT ROOM 2B		No.2 to No.3	No.3 TREATMENT ROOM 2C	
	GQ22A	GQ24A	GQ19	GQ22B	GQ24B	GQ20	GQ22C	GQ24C
70	...	...	...	...	...	...	...	...
80	...	...	...	...	...	...	...	...
90	...	...	...	...	...	...	...	...
⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮
⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮
⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮	⋮

ENERGY (MeV)	No.3 to No.4	No.4 TREAT- MENT ROOM 3	SWITCHING POWER SOURCE 162-1	SWITCHING POWER SOURCE 162-2	SWITCHING POWER SOURCE 162-3	SWITCHING POWER SOURCE 162-4
	GQ27	GQ28				
70	...	...	...	...	...	...
80	...	...	...	...	...	...
90	...	...	...	...	...	...
⋮	⋮	⋮	⋮	⋮	⋮	⋮
⋮	⋮	⋮	⋮	⋮	⋮	⋮
⋮	⋮	⋮	⋮	⋮	⋮	⋮



# FIG.9

GB : BENDING ELECTROMAGNET

GQ : QUADRUPOLE ELECTROMAGNET

TREAT- MENT ROOM No.	COMMON						
	BEFORE ACCELERATION		SYNCHROTRON			AFTER ACCELERATION	
	GB10	GQ9	GB14	GQ13	GQ13	GB17	GQ18
1	ON						
2							
3							
4							

TREAT- MENT ROOM No.	No.1 TREATMENT ROOM 2A		No.1 to No.2	No.2 TREATMENT ROOM 2B		No.2 to No.3	No.3 TREATMENT ROOM 2C	
	GQ22A	GQ24A		GQ19	GQ22B		GQ24B	GQ20
1	ON		No Care					
2	No Care		ON	ON		No Care		
3	No Care		ON	No Care		ON	ON	
4	No Care		ON	No Care		ON	No Care	

TREAT- MENT ROOM No.	No.3 to No.4	No.4 TREAT- MENT ROOM 3	SWITCHING POWER SOURCE 162-1	SWITCHING POWER SOURCE 162-2	SWITCHING POWER SOURCE 162-3	SWITCHING POWER SOURCE 162-4
	GQ27	GQ28				
1			ON			
2						
3	No Care					
4	ON	ON				

# FIG.10

GB : BENDING ELECTROMAGNET  
GQ : QUADRUPOLE ELECTROMAGNET

PATIENT ID No.	DOSE ROOM No.	TREAT- MENT ROOM No.	ENERGY	COMMON					
				BEFORE ACCELERATION		SYNCHROTRON		AFTER ACCELERATION	
				GB10	GQ9	GB14	GQ13	GQ13	No.1 TREATMENT ROOM 2A
650098	...	No.1	70Mev	...	...	Pattern 70		...	...
									...

		No.1 to No.2	No.2 TREATMENT ROOM 2B	No.2 to No.3	No.3 TREATMENT ROOM 2C	No.3 to No.4	No.4 TREATMENT ROOM 3
	GQ19	GQ22B	GQ24B	GQ20	GQ22C	GQ24C	GQ28
	No Care	No Care	No Care	No Care	No Care	No Care	No Care

		SWITCHING POWER SOURCE 162-1	SWITCHING POWER SOURCE 162-2	SWITCHING POWER SOURCE 162-3	SWITCHING POWER SOURCE 162-4
	...	...	...	...	...

FIG.11

GB : BENDING ELECTROMAGNET

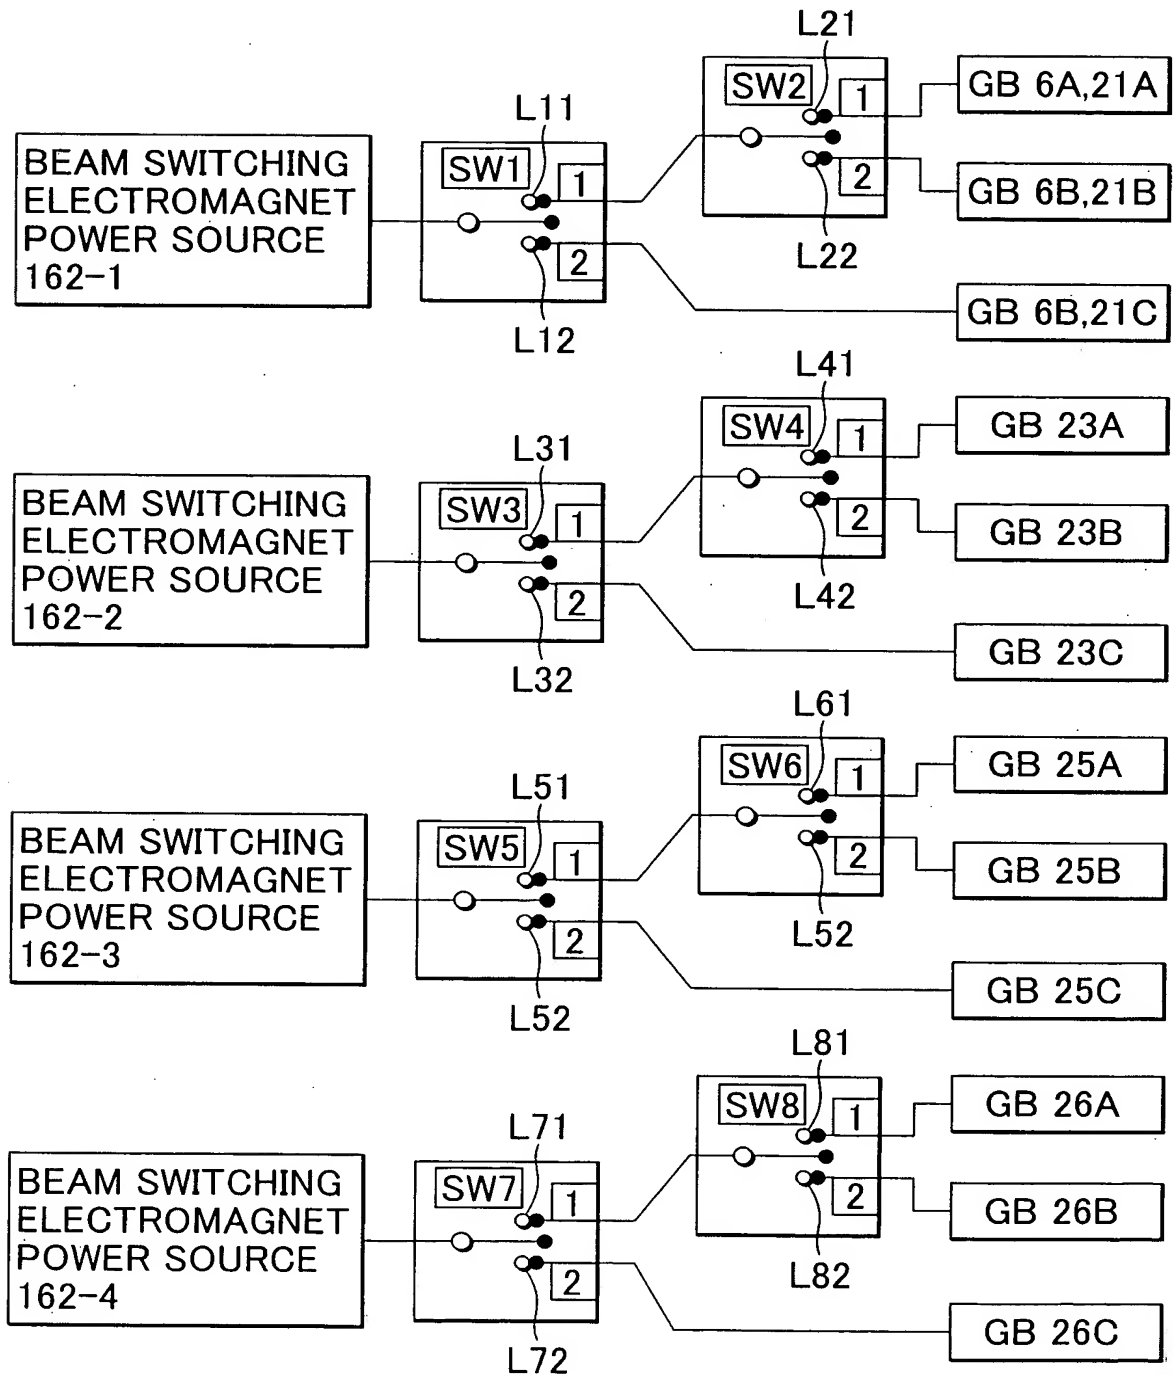


FIG.12

[illegible]

# FIG.13

<REFERENCE CONFIGURATION DATA>

PATIENT ID No.	DOSE	TREATMENT ROOM No.	ENERGY
650098	...	No.1	70MeV

COMMON									
BEFORE ACCELERATION			SYNCHROTRON			AFTER ACCELERATION			No.1 TREMENT ROOM 2A
GB10	...	Q9	GB14	Q13	Q13	GB17	Q18	Q24A	...
...	...	...	Pattern 70			...	...	...	...

No.1 to No.2	No.2 TREATMENT ROOM 2B	No.2 to No.3	No.3 TREATMENT ROOM 2C	No.3 to No.4	No.4 TREATMENT ROOM 3
Q19	Q22B	Q24B	Q20	Q22C	Q24C
No Care	No Care	No Care	No Care	No Care	No Care

GB : BENDING ELECTROMAGNET  
 GQ : QUADRUPOLE ELECTROMAGNET

SWITCHING POWER SOURCE 162-1	SWITCHING POWER SOURCE 162-2	SWITCHING POWER SOURCE 162-3	SWITCHING POWER SOURCE 162-4
...	...	...	...


B (6)

A (5)

5



FIG.15

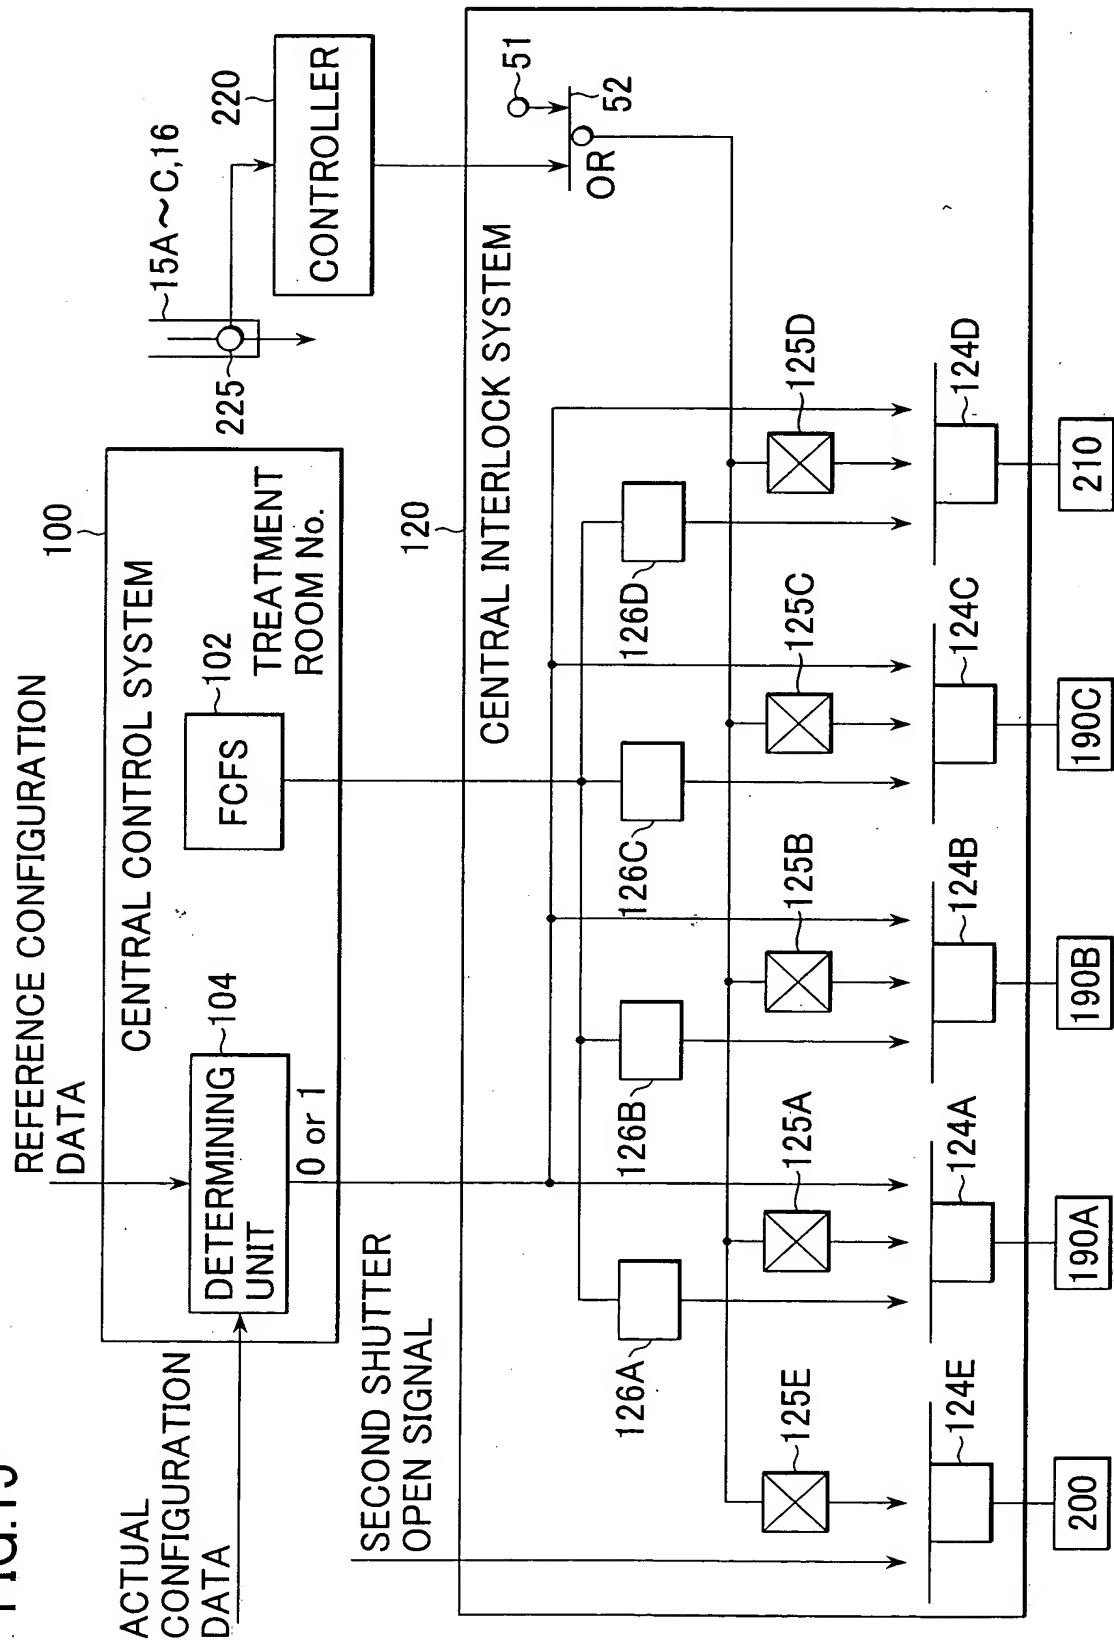

# FIG.16

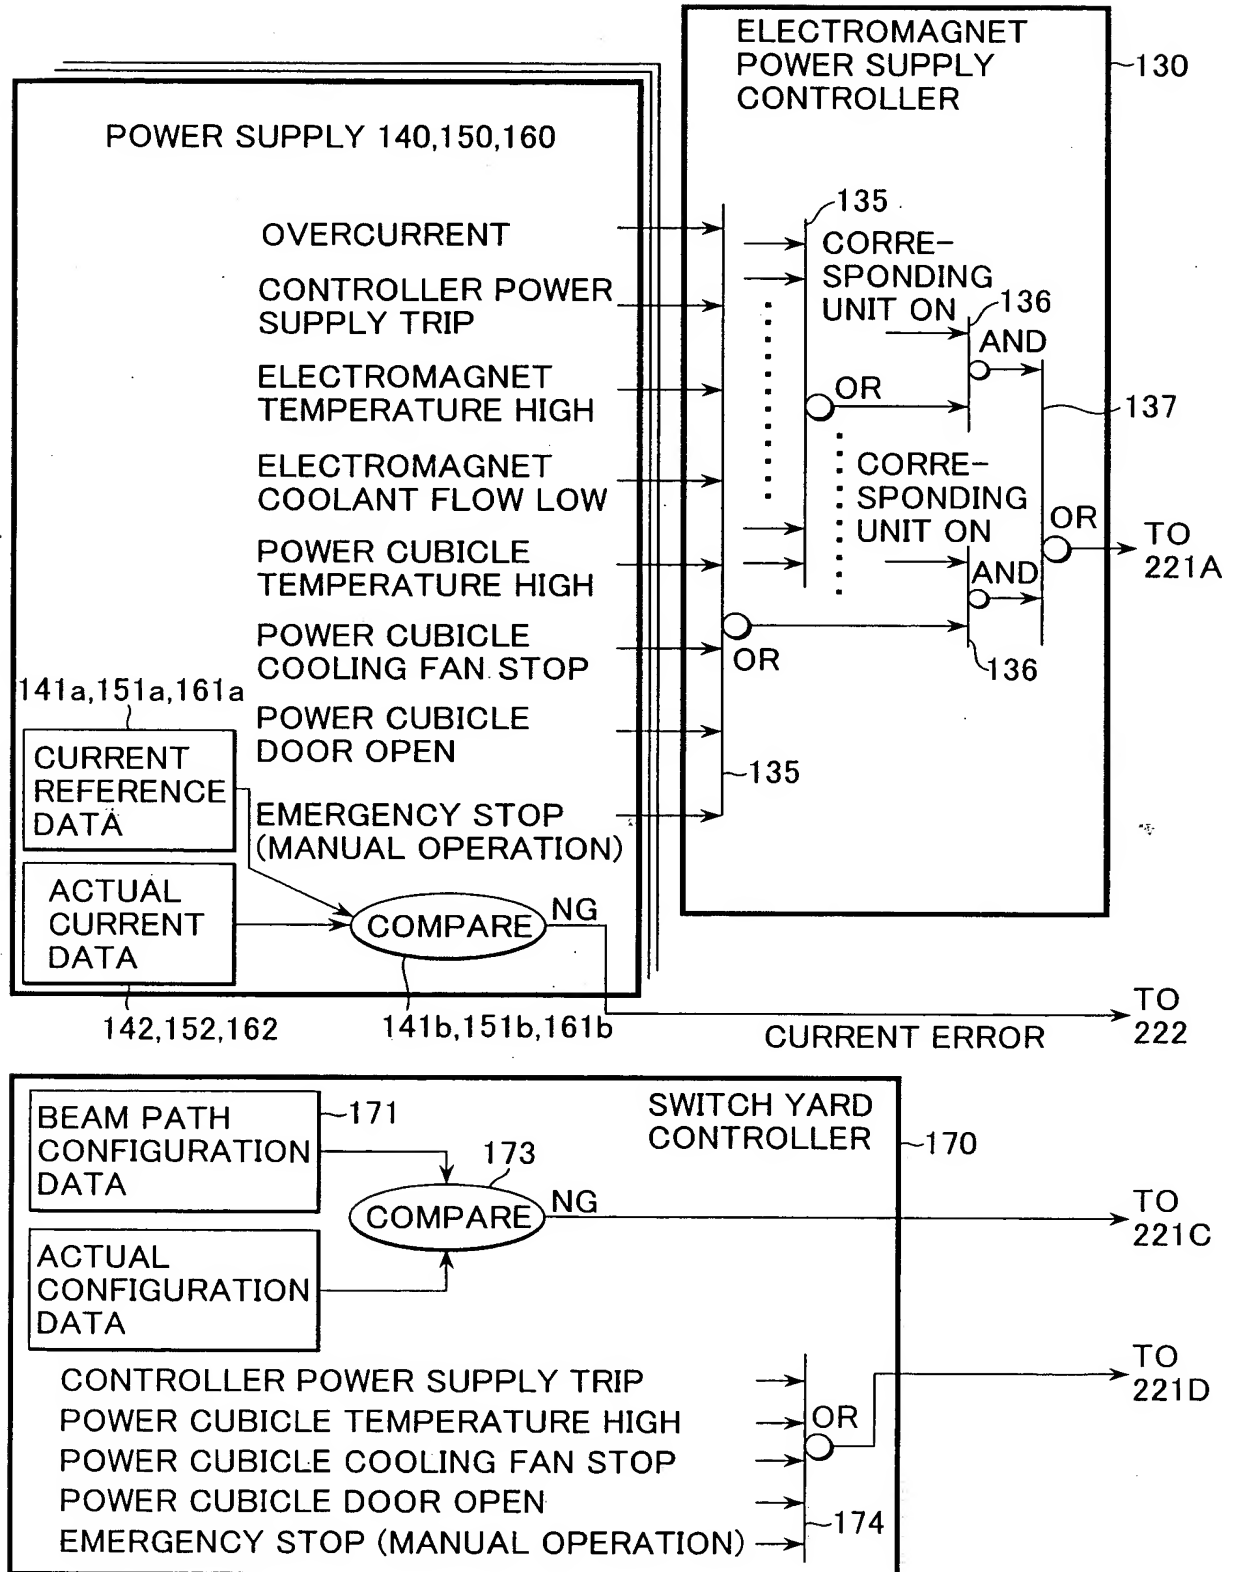




FIG.17

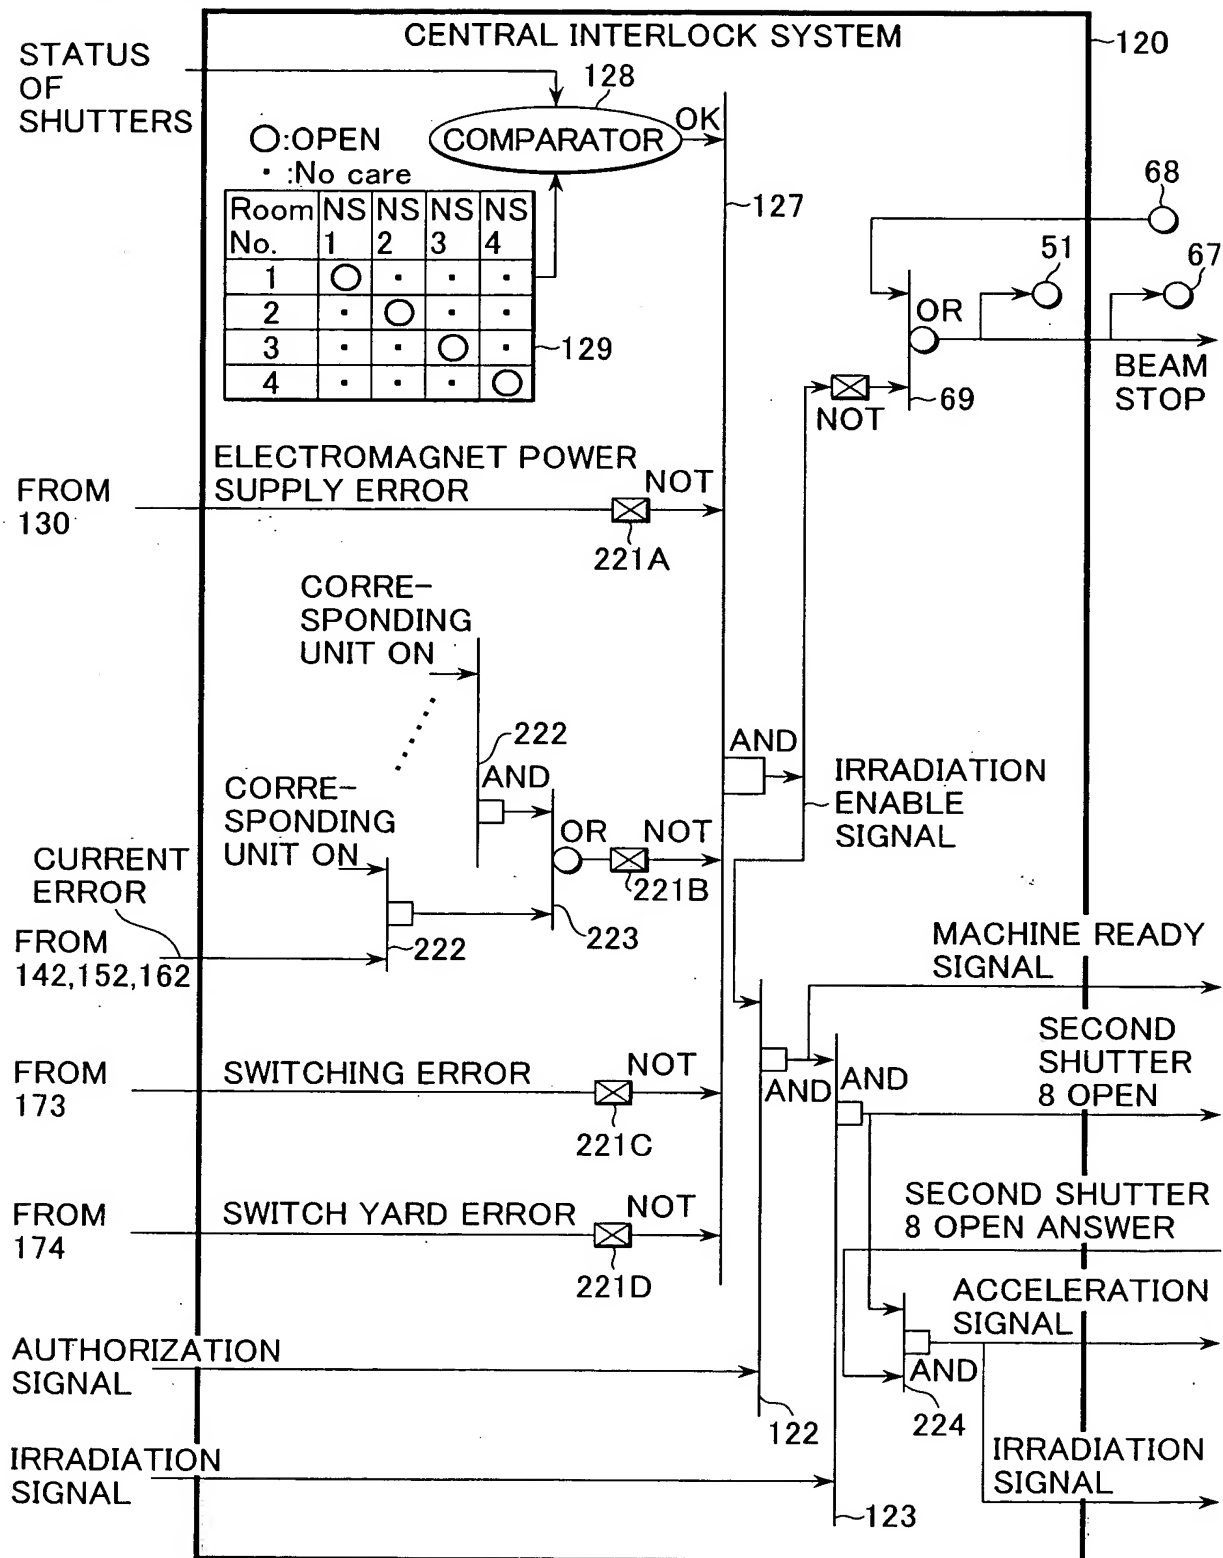


FIG.18

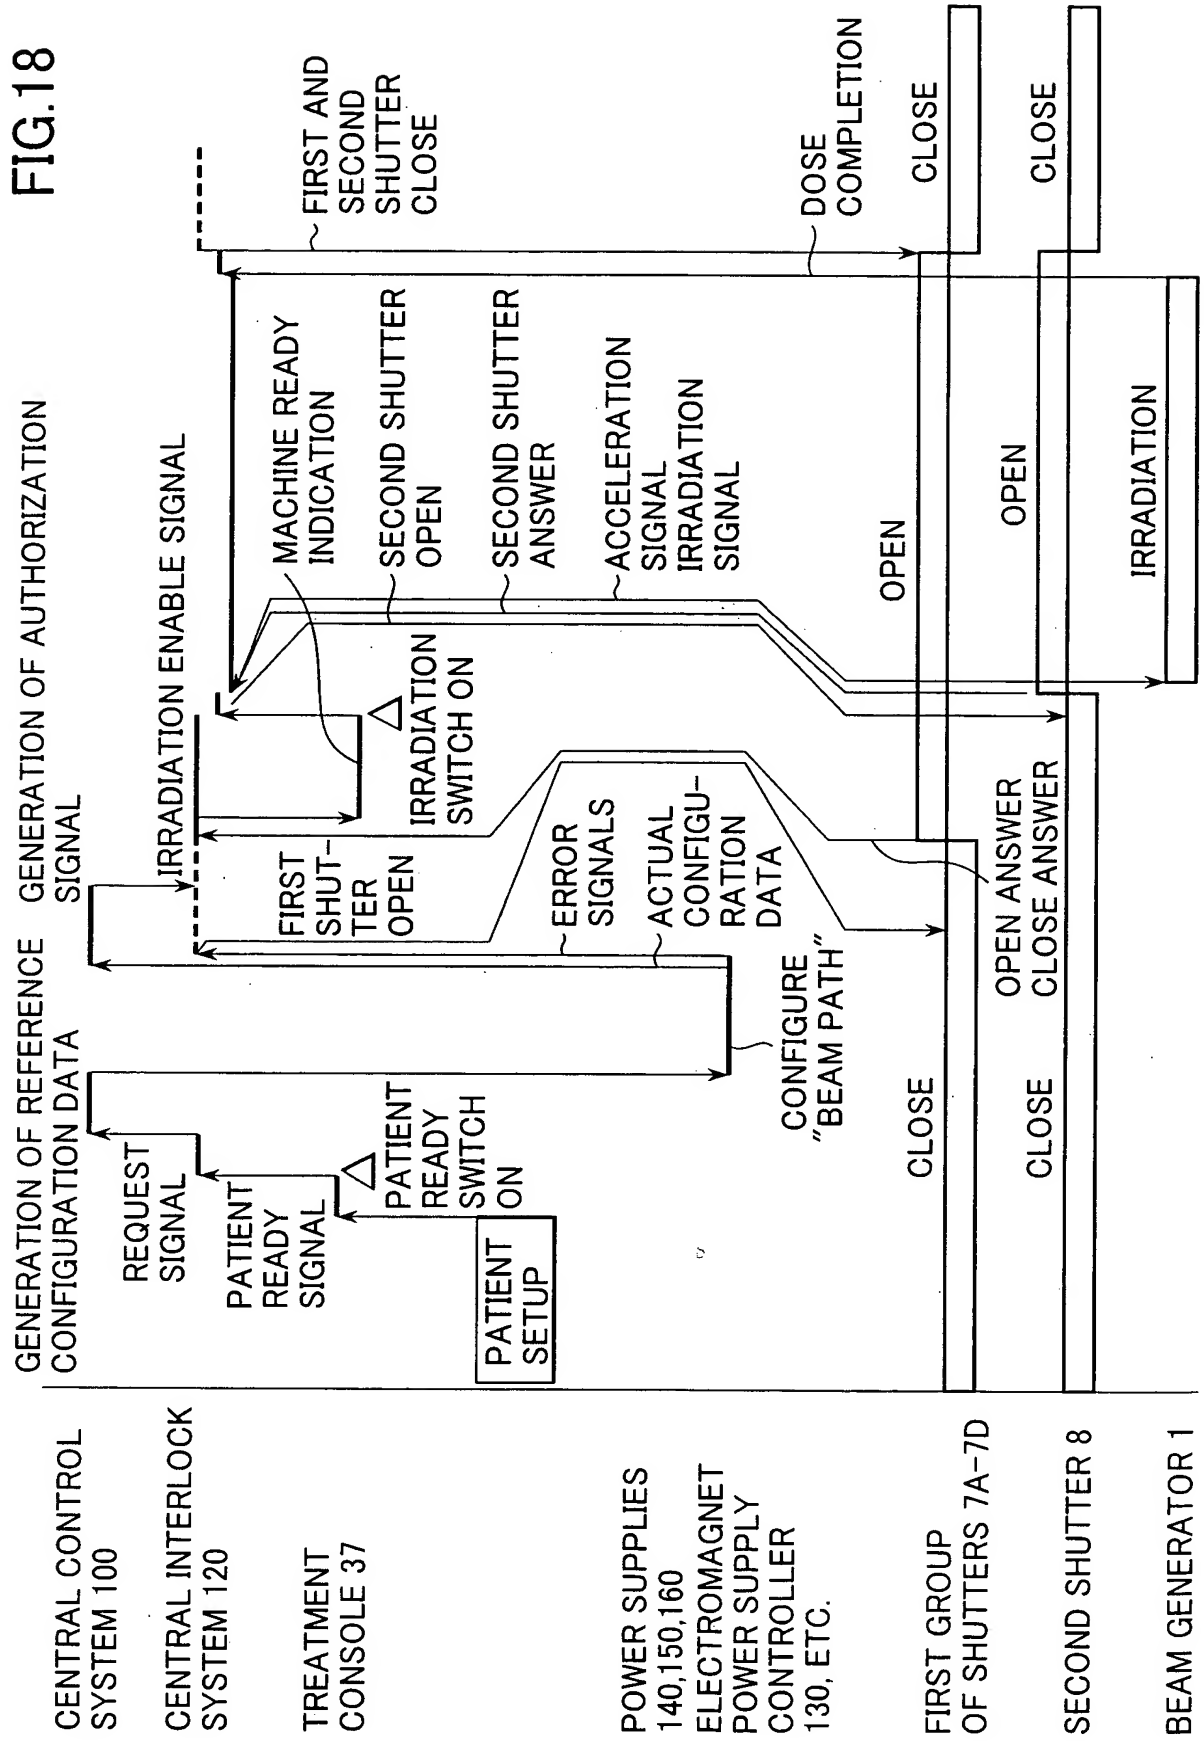


FIG.19

GB : BENDING ELECTROMAGNET

